

UniLine ACID Storage Cabinets



- Molded one piece chemical and acid resistant, composite liner, molded one-piece covered corners, glass smooth for ease of cleaning
- Cabinet Exhaust can be vented out the back or through the fume hood or through an exhaust blower system
- Removable rear panel allows access to connect venting
- Removable Shelf for small container storage
- Front Access doors are lined and edges are sealed
- Door Vents provide Supply air ventilation
- Removable containment tray
- Containment Lip on front bottom edge of cabinet to hold spills

For storage of ACID and corrosive chemicals, available in 12", 18", 24", 30", 36", 42" & 48" widths. Standard 35 1/4" high and 22" deep cabinet dimension. (as shown) U.L. 1805 Fume Hoods & Cabinets. Cabinets are designed to hold specific chemicals




Optional Acid Storage Containment Tray to contain spillage and provides ease of cleanup. (located in bottom of cabinet)



18"-24" Left Hinged

18"-24" Right Hinged

30"-48"

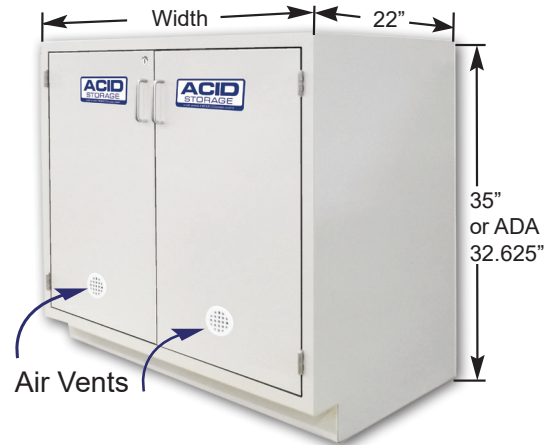


Air Vents


Acid Cabinet Size							
Width	12"	18"	24"	30"	36"	42"	48"
35 1/4" high X 22" deep	15120	15180	15240	15300	15360	15420	15480

Venting Your Acid Cabinet (select 1 or 2)

- ① Acid Cabinet Vent Through Fume Hood Double Side Wall & worksurface
- (1) 90 Degree Elbow
(1) Vent outlet Exhaust Vent Kit
Cat. No. 81001

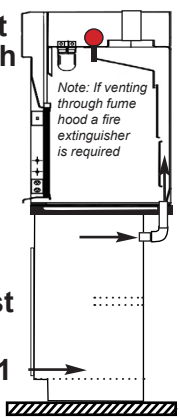

- ② Acid Cabinet Exhaust Blower through the wall
- (1) 90 Degree Elbow Exhaust
(1) 10' Ridge & Flex
(1) Exhaust Blower Vent Outlet
Cat. No. 81002

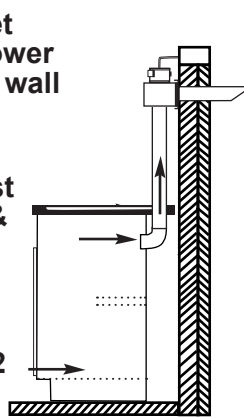

Liquid Chemical Storage Cabinets shall be in an area of the laboratory with low traffic away from the main work area. It is important to segregate incompatible chemicals. Eliminate ignition sources such as open flame, hot surfaces, electrical equipment or static electricity from the storage area. Make sure appropriate fire extinguishers and/or sprinkler systems are in the area. An eyewash and safety shower must be readily accessible to areas where liquid chemicals are stored, per OSHA 1910.106(d)(3)(I).

Note: Venting voids the U.L. listing, If applicable, as site conditions cannot be verified by U.L.

